


RHEOMETER REPORT

XYZ

TEMP(C)	160.0
TIME(MIN)	4.0
TORQUE UNIT	kgf*cm

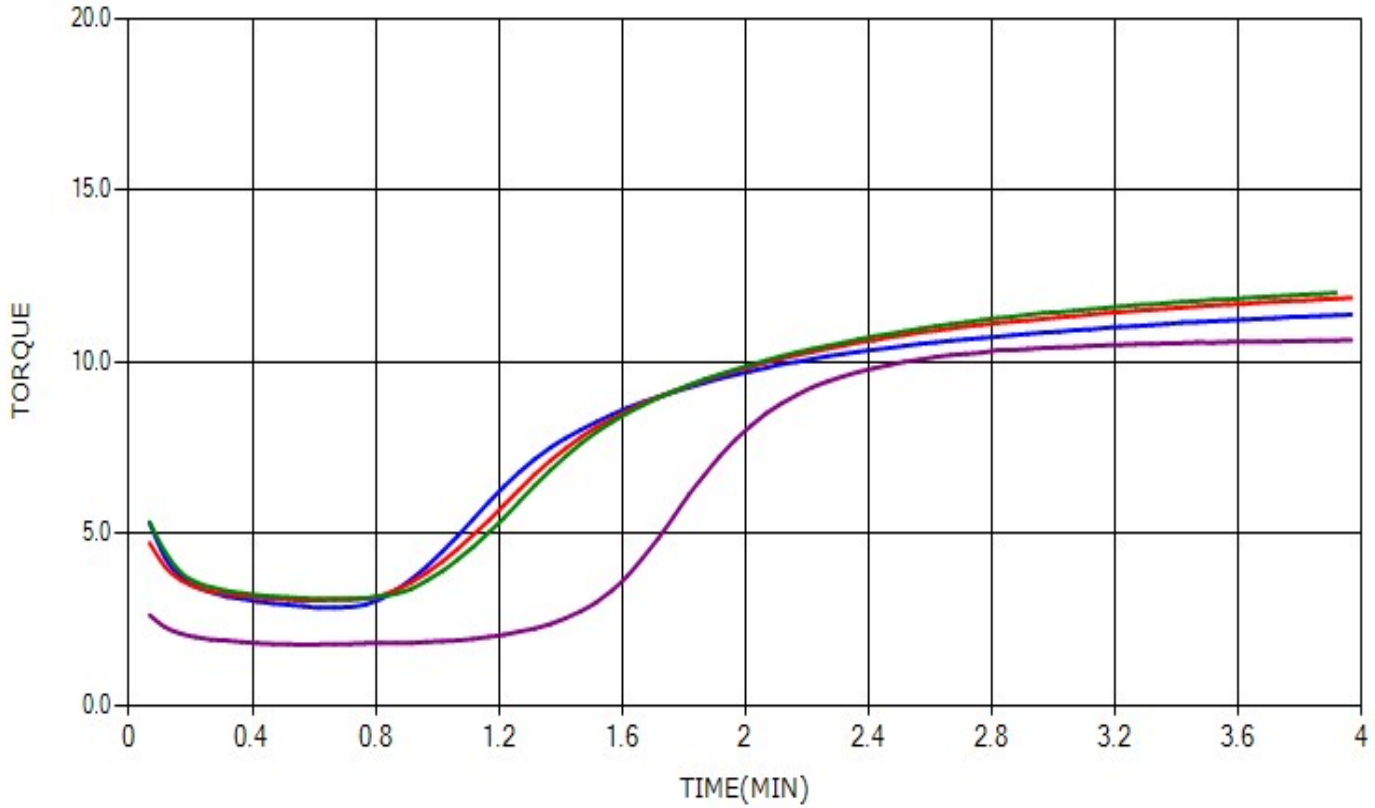

ID1	ID2	ID3	QC	ML	MH	ts1	ts2	tc10	tc50	tc90	Date
999			OK	2.85	11.39	0.93	1.05	0.92	1.30	2.55	2016/04/08 14:01:57
789			OK	3.05	11.88	0.98	1.12	0.97	1.40	2.68	2016/04/07 16:42:18
567			OK	3.10	12.04	1.03	1.17	1.02	1.45	2.70	2016/04/07 16:35:38
345			OK	1.77	10.66	1.47	1.60	1.43	1.82	2.38	2016/04/06 11:10:03

Lower Limit	1.50							1.05		
Upper Limit								1.95		
Average	2.69	11.49	1.10	1.23	1.08	1.49	2.58			
Standard deviation	0.62	0.62	0.25	0.25	0.24	0.23	0.15			
Coefficient of variation(%)	23.09	5.42	22.20	20.20	21.87	15.11	5.69			